



Morgan Scientific, Inc.

PFT Laboratory

**151 Essex Street
Haverhill, MA 01832
(978) 521-4440**

Date: **28-Dec-05**

Temp: 22°C

Pressure: 768mmHg

Humidity: 50%

BTPS: 1.109

Name: **Michael J. Callahan**

DOB: **02-Jul-53**

Age: **52**

ID #: **09413352**

Sex: **M**

Height: **70 in**

Weight: **275 lb**

Technician: **Patrick Morgan**

Race: **W**

Smoker: **N**


Pack years: **N/A**

Referring Physician: **John Williams, M.D.**

Spirometry

Parameter	Units	Predicted	Observed		Observed		Percent Change
		Value	Pre	% Pred	Post	% Pred	
FVC	L	5.02	4.35	87	4.33	86	0
FEV1	L	3.88	3.31	85	3.19	82	-4
FEV1 / FVC	%	77	76	99	74	96	-3
FEF@%	L/s	8.23	7.90	96	7.49	91	-5
FEF%)	L/s	4.73	3.95	84	3.49	74	-12
FEF&%	L/s	1.84	0.86	47	0.56	30	-35
FEF@%_&%	L/s	3.38	2.76	82	2.26	67	-18
PEFR	L/s	9.74	8.54	88	8.44	87	-1
FIF50	L/s	----	5.96	----	6.24	----	5
PIFR	L/s	6.49	5.98	92	6.34	98	6
FIVC	L	5.02	4.02	80	4.17	83	4
FET	sec	----	10.33	----	13.80	----	34
MVV	L/m	151.6	----	----	----	----	--

Flow Volume

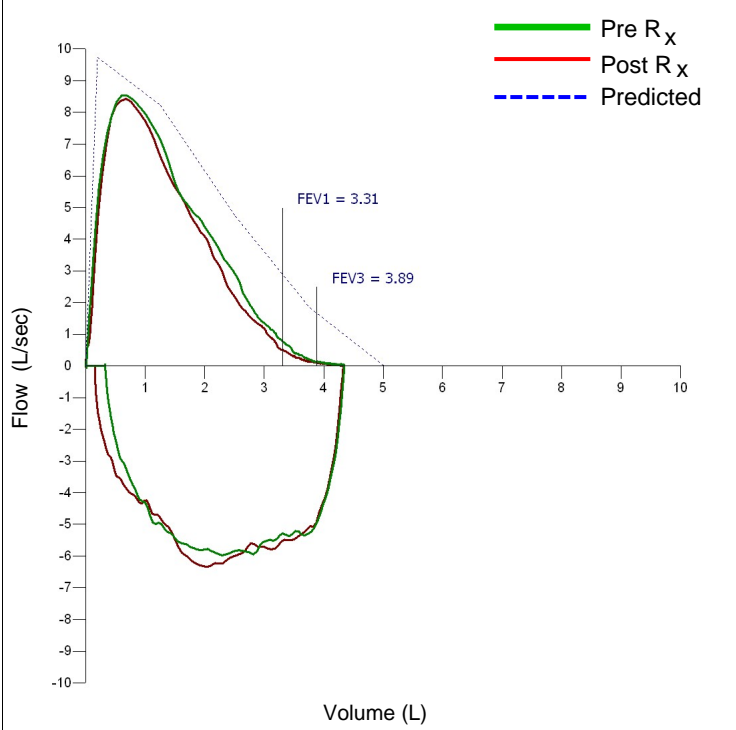

Technician Notes:

Patient was very cooperative

Physician Interpretation

These test results indicate normal pulmonary function.

Signed: _____

Colin Chapman, M.D.